

# 迪西吸入研发服务平台

&

(Orally Inhaled Drug Products ODPs)

/

(COPD)



(DPI)



(Nebulizer)



(MDI)



(Inhalation Sprays)



(Dry Powder Inhaler, DPI)



- pH
- 

- /
- / /

- /
- 

|   | ) | ) | ) | ) | ) |
|---|---|---|---|---|---|
| - | ) | + | + | + | ) |
|   | ) | + | + | ) | ) |
|   | + | ) | ) | ) | ) |
|   | + | ) | ) | ) | ) |
|   | + | + | + | ) | ) |



DPI-




DPI-



MDI-

-DPI/MDI

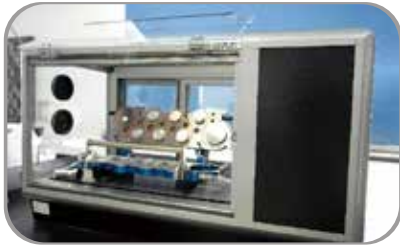

+



+

-




+



DUSA +



+

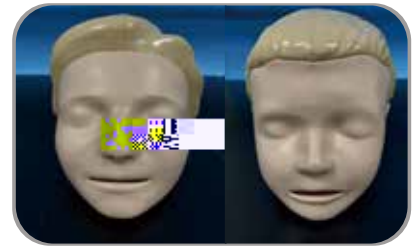

+



+

COPLEY

(NGI) COPLEY

BRS2100

NGI

Inhalytix

ICH

qqPL? 5.

/.




Waters ACQUITY H-class-QDA


IC (Thermo Aquion RFIC )

SHIMADUZ/GC-2010plus



AKA

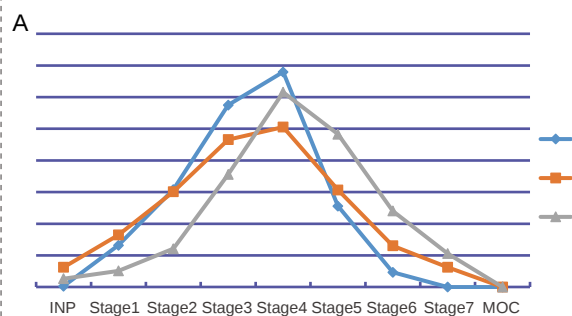

A

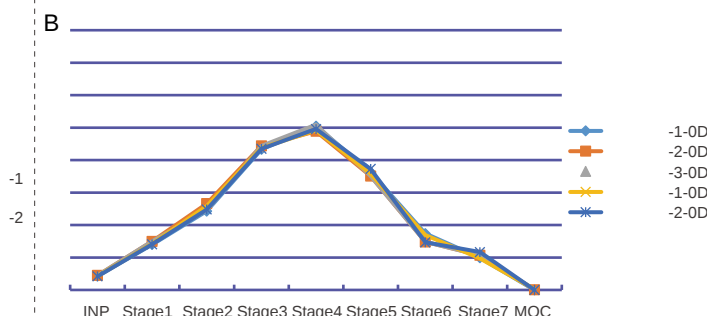

B)

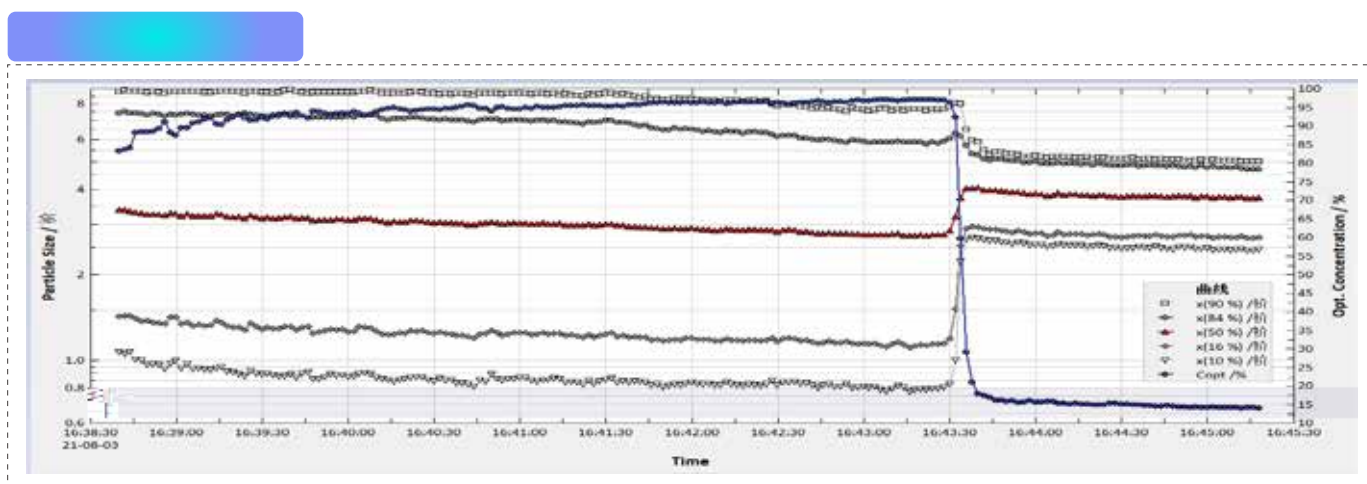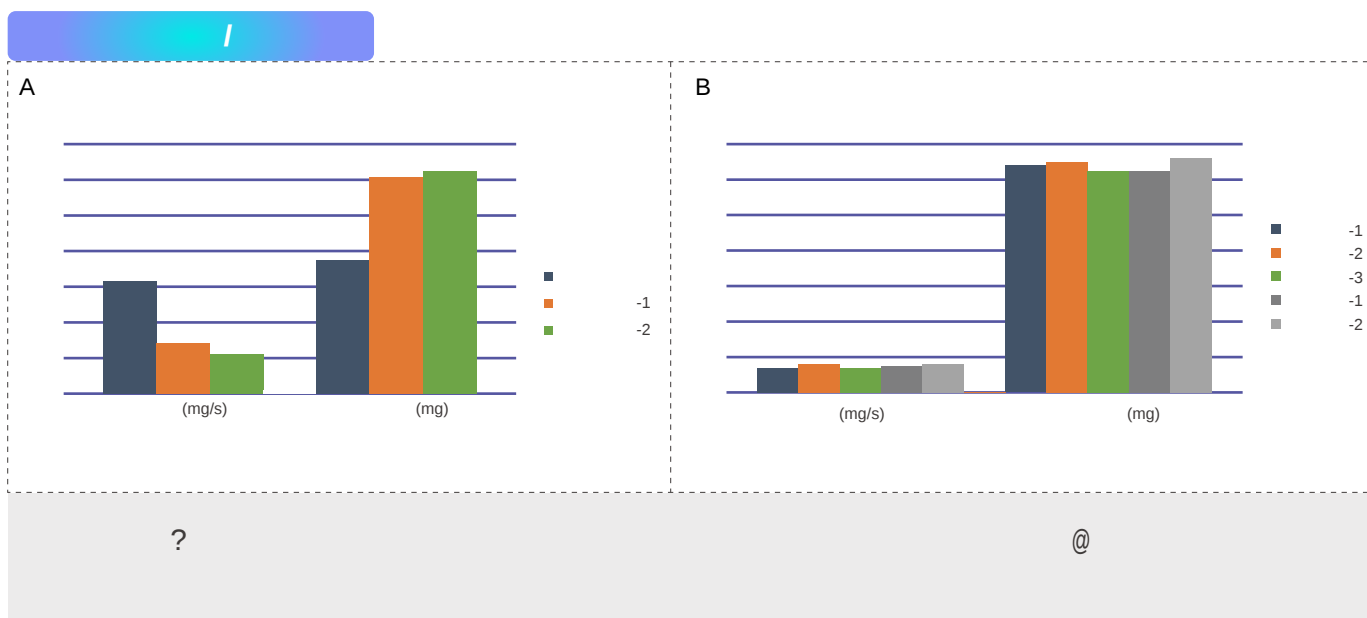

|    | D10 $\mu\text{m}$ | D50 $\mu\text{m}$ | D90 $\mu\text{m}$ | 0.5~5 $\mu\text{m}$ % |
|----|-------------------|-------------------|-------------------|-----------------------|
| -1 | 1.11              | 3.36              | 9.92              | 65.58                 |
| -2 | 1.13              | 3.48              | 9.83              | 66.23                 |
| -1 | 1.05              | 3.52              | 9.78              | 67.52                 |
| -2 | 1.09              | 3.39              | 9.98              | 66.13                 |

1 4

/

- 
- 
- 
- 

OECD  
4

5

28

90

- 
- 
- 
- 
- 
- 

28

90

2 2

|  | <ul style="list-style-type: none"><li></li><li></li><li></li><li></li></ul>                   |  |  |  |
|--|-----------------------------------------------------------------------------------------------|--|--|--|
|  | <ul style="list-style-type: none"><li></li><li></li><li></li><li></li><li></li><li></li></ul> |  |  |  |
|  | <ul style="list-style-type: none"><li></li><li></li><li></li></ul>                            |  |  |  |

GLB



400-780-8018  
www.medicilon.com.cn  
marketing@medicilon.com.cn  
585

1. 样品发生模块



液体气溶胶发生器



粉尘气溶胶发生器



MDI

3. 分析模块



暴露环境监测



气溶胶浓度监测



粒径分布监测

2. 染毒模块



4. 控制模块



计算机和软件

5. 废气处理模块



控制柜

1. 样品发生模块



液体气溶胶发生器



粉尘气溶胶发生器

3. 分析模块



暴露环境监测



气溶胶浓度监测



粒径分布监测

2. 染毒模块



4. 控制模块




计算机和软件

5. 废气处理模块



控制柜



•  
•

•  
•  
•  
•

/

PK

•  
•  
•  
•  
•

/

•  
•  
•

CMC